



TELIC LABS

MEDICAL GRADE CBD AND HEMP PRODUCTS DESERVE
MEDICAL GRADE TESTING

LABORATORY CERTIFICATION OF ANALYSIS:


| Sample Information | |
|--------------------|-----------------------|
| Client ID: | TZV-0606 |
| Accession ID: | 22154003 |
| Sample ID: | CG-22518-001 |
| Sample Matrix: | Infused Product - Oil |
| Date Received: | 06/03/2022 |

| Client Information | |
|----------------------|--|
| Name / Business | Green County Hemp |
| Address: | 1810 Wright Street |
| City/State/Zip Code: | Madison, WI 53704 |
| Phone Number: | (608) 622-4021 |
| Email Address: | brook@greencountyhemp.com |





| | | |
|-------------------------------------|------------------------------|----------------------|
| Cannabinoid Profile Analysis | Test Date: 06/06/2022 | Tested By: BK |
|-------------------------------------|------------------------------|----------------------|

Infused Products are analyzed via HPLC-UV by mass with comparison to certified reference standards at known concentrations.

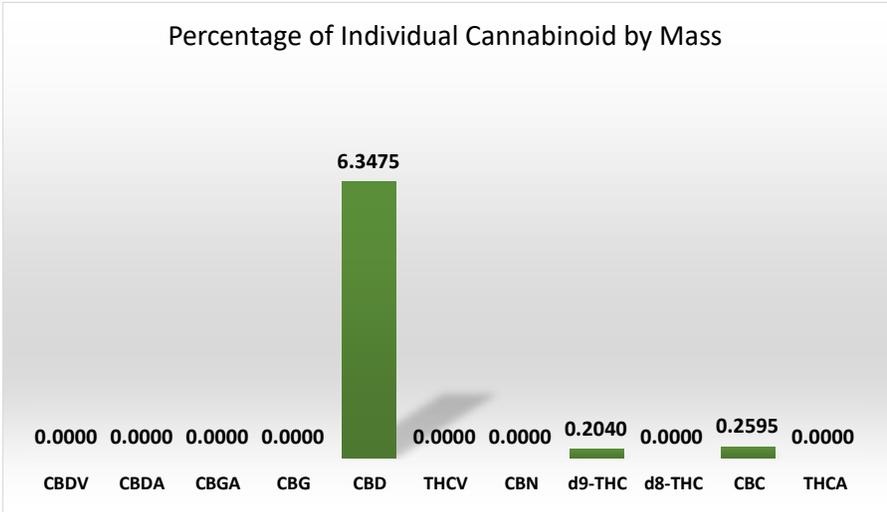

| Cannabinoid | Conc. (mg/mL) |
|------------------------------------|---------------|
| CBDV | 0.000 |
| CBDA | Not Detected |
| CBGA | Not Detected |
| CBG | Not Detected |
| CBD | 63.475 |
| THCV | Not Detected |
| CBN | Not Detected |
| d9-THC | 2.040 |
| d8-THC | Not Detected |
| CBC | 2.595 |
| THCA | Not Detected |
| Total Cannabinoids | 68.110 mg/mL |
| | 6.81 % |
| Density Factor | 1.00 |
| Total CBD : Total THC Ratio | |
| 31.11 :1 | |

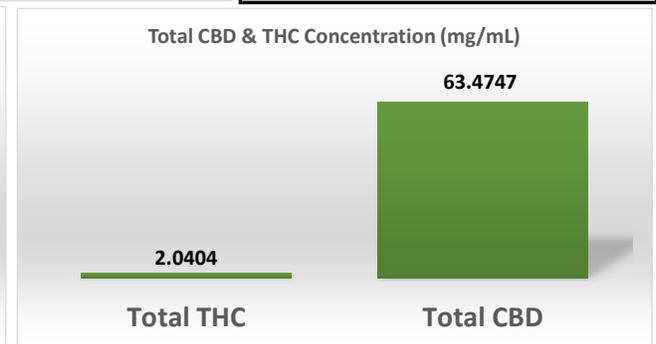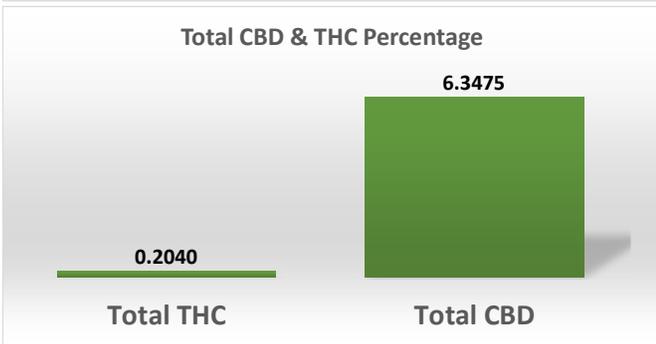

Comments:
 Density not measured.
 Moisture content assay not performed on this sample matrix.
 Cultivar/Batch/Lot:

Notes & Disclaimers:
 1) Total THC = d9-THC+(THCA*0.877), Total CBD = CBD+(CBDA*0.877).
 2) DBNQ = Detected but not quantifiable.
 3) These results relate only to the test article listed in this report. Reports may not be reproduced except in their entirety.
 4) All results apply to the samples as received. Improper collection of samples can affect the validity of results and is not the responsibility of the lab.
 5) Density factor is an estimate unless exact density is provided to lab. If base matrix type is not provided an estimated value of 1.0g/mL will be used.

| | | | | | |
|----------------------|-----------------|------------|-----------------------|-------|------------|
| Results Verified By: | Josh Smith M.S. | Signature: | <i>Joshua A Smith</i> | Date: | 06/07/2022 |
|----------------------|-----------------|------------|-----------------------|-------|------------|